


Provided for non-commercial research and education use.
Not for reproduction, distribution or commercial use.

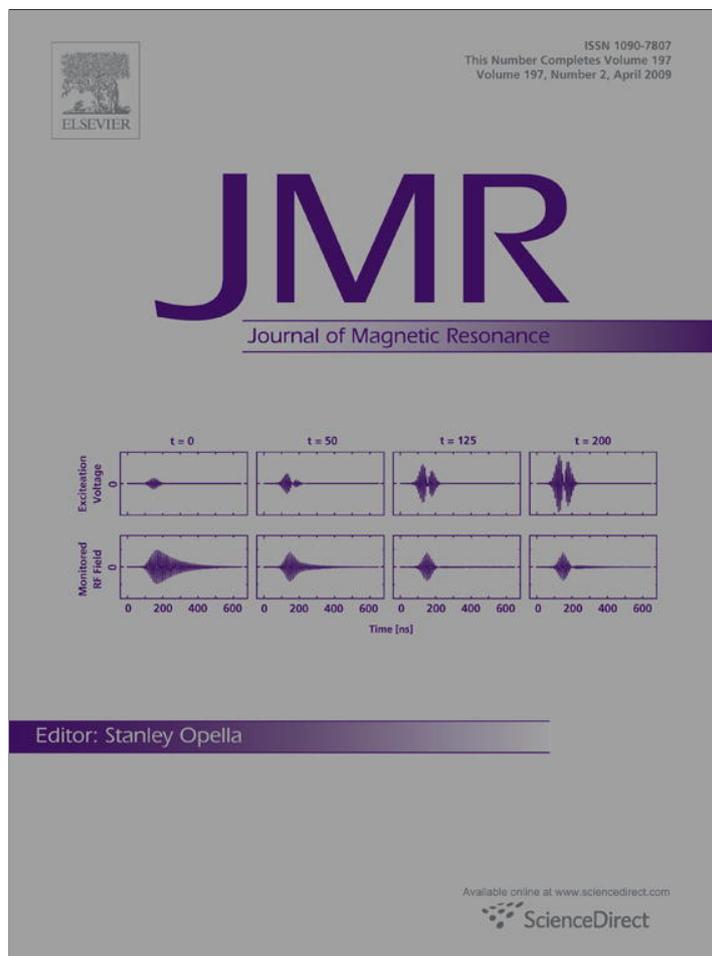

This article appeared in a journal published by Elsevier. The attached copy is furnished to the author for internal non-commercial research and education use, including for instruction at the authors institution and sharing with colleagues.

Other uses, including reproduction and distribution, or selling or licensing copies, or posting to personal, institutional or third party websites are prohibited.


In most cases authors are permitted to post their version of the article (e.g. in Word or Tex form) to their personal website or institutional repository. Authors requiring further information regarding Elsevier's archiving and manuscript policies are encouraged to visit:

<http://www.elsevier.com/copyright>



Contents lists available at ScienceDirect

Journal of Magnetic Resonance

journal homepage: www.elsevier.com/locate/jmr

Nano-emulsions of fluorinated trityl radicals as sensors for EPR oximetry

N. Charlier^a, B. Driesschaert^{a,b}, N. Wauthoz^d, N. Beghein^a, V. Pr at^c, K. Amighi^d,
J. Marchand-Brynaert^b, B. Gallez^{a,*}^a *Universit  catholique de Louvain, Laboratory of Biomedical Magnetic Resonance, REMA, Avenue Mounier 73.40, B-1200 Brussels, Belgium*^b *Universit  catholique de Louvain, Organic and Medicinal Chemistry Unit, Louvain-la-Neuve, Belgium*^c *Universit  catholique de Louvain, Pharmaceutical Technology Unit, Brussels, Belgium*^d *Universit  libre de Bruxelles, Laboratory of Pharmaceutics and Biopharmaceutics, Universit  libre de Bruxelles, Brussels, Belgium*

ARTICLE INFO

Article history:

Received 27 August 2008

Revised 24 November 2008

Available online 24 December 2008

Keywords:

EPR

In vivo

Oximetry

Biocompatibility

ABSTRACT

This article reports the development and evaluation of two nano-emulsions (F45T-03/HFB and F15T-03/PFOB) containing fluorinated trityl radicals dissolved in perfluorocarbons. Preparation with a high-pressure homogenizer conferred sub-micronic size to both nano-emulsions. In vitro and in vivo EPR spectroscopy showed that the nano-emulsions had much greater oxygen sensitivity than the hydrophilic trityl, CT-03. In vivo experiments in rodents confirmed the ability of the nano-emulsions to follow the changes in oxygen concentration after induced ischemia. Histological evaluation of the tissue injected with the nano-emulsions revealed some acute toxicity for the F45T-03/HFB nano-emulsion but none for the F15T-03/PFOB nano-emulsion. These new formulations should be considered for further EPR oximetry experiments in pathophysiological situations where subtle changes in tissue oxygenation are expected.

  2008 Elsevier Inc. All rights reserved.

1. Introduction

The role played by oxygen in physiopathological processes and therapeutics is of crucial importance. The development of non-invasive tools for monitoring tissue oxygenation may have profound diagnostic and therapeutic implications in oncology and in cardiovascular diseases. Existing methods for estimating pO_2 in tissues include magnetic resonance (MR)-based and non-MR-based techniques. Non-MR-based oximetry methods include polarographic oxygen electrodes, fluorescence quenching, phosphorescence quenching, near infra-red spectroscopy (NIRS), and the use of bioreductive markers selectively trapped in hypoxic regions. MR-based techniques include ^{19}F -NMR spectroscopy/imaging, blood oxygen level-dependent (BOLD) NMR imaging, electron paramagnetic resonance (EPR) spectroscopy/imaging, and dynamic nuclear polarization (DNP) which involves both NMR and EPR (for a review, see [1–3]).

In EPR oximetry, the oxygen content in tissues is measured by the effect of oxygen on the EPR spectrum of a paramagnetic oxygen sensor. These oxygen sensors can be classified into two groups: Particulate paramagnetic materials and soluble paramagnetic materials. The particulate probes include lithium phthalocyanine [4] and naphthalocyanine crystals [5], natural charcoals [6,7], analytical charcoals [8,9], India inks [10,11], and carbon blacks [12]. These materials possess high sensitivity to changes in oxygen con-

centration (large variation in EPR line width [LW] as a function of the pO_2), in vivo inertness, and a high spin density providing a high signal-to-noise ratio (SNR). However, for imaging applications, it may be interesting to use soluble probes that can diffuse inside tissues and provide information about the spatial distribution of oxygen within a tissue. Among soluble materials, two types of structure are particularly interesting: The nitroxides and the triarylmethyl (trityl or TAM) radicals. Various chemical properties of the nitroxides can be manipulated to modulate intracellular accumulation or tissue selectivity [13,14]. Nitroxides are metabolically converted to the EPR-silent hydroxylamines. Trityls are characterized by a narrower LW and a higher stability compared to nitroxides [15]. Trityls have been used as oxygen/pH probes [16–20], and as contrast agents in EPR [21] and DNP [22,23] imaging. Soluble paramagnetic probes are less sensitive to oxygen changes compared to particulate probes. This limited sensitivity to oxygen can be problematic for evaluating subtle changes in tissue oxygenation. To overcome this limitation, Liu and colleagues proposed encapsulating nitroxides in lipophilic environments [24]. Consistent with the Smoluchowski equation, as oxygen is more soluble in lipophilic environments than in water, an increase in sensitivity can be achieved using these systems. For this proof-of-concept, Liu et al. used nitroxides dissolved in common organic solvents and encapsulated in denatured albumin microspheres with a size of 2.5 μm . More recently, Kuppusamy's group reported the synthesis [25] and use of a trityl radical (perchlorotriphenyl methyl-triester radical or PTM-TE in HFB). The authors also used bovine serum albumin (BSA) in order to encapsulate a solution of PTM-TE

* Corresponding author. Fax: +32 2 7647390.

E-mail address: bernard.gallez@uclouvain.be (B. Gallez).

dissolved in HMDS [26]. HFB belongs to the class of perfluorocarbons (PFC) that have very high oxygen solubility. PFCs are able to dissolve up to about 50% their volume of oxygen [27].

It could be desirable to extend this concept to other PFCs which are biocompatible and already used clinically as blood substitutes (e.g., perfluorooctyl bromide (PFOB)). Moreover, it could be interesting to use a biocompatible nano-capsule as a vehicle, because BSA can generate immunogenic responses [28]. Furthermore, a nano-size formulation is suitable for parenteral administration and decreases uptake by the reticuloendothelial system after intravenous administration. To achieve these goals, we sought to enhance the affinity of the oxygen spin probe for a PFC formulation by attaching a perfluorinated tag on trityl radicals [29]. Introducing a fluorine label on a molecule enhances its fluorophilicity [30]. Two new trityl radicals (Fig. 1), called F15T-03 and F45T-03 (which contain three fluorine chains with 5 and 15 fluorine atoms, respectively), were recently synthesized by our group [29]. These radicals exhibit a single, sharp EPR spectrum. Calibration was performed in PFC solvents according to the respective solubility of the compounds. The oxygen sensitivities of F15T-03 in HFB and F45T-03 in PFOB were 1.87 $\mu\text{T}/\text{mm Hg}$ and 1.75 $\mu\text{T}/\text{mm Hg}$, respectively [29]. This sensitivity was markedly increased compared to the hydrophilic trityl, CT-03 (0.064 $\mu\text{T}/\text{mm Hg}$). The aim of the present work was to develop and optimize the preparation of nano-emulsions containing these fluorinated trityls included in PFC solvents. These new oxygen sensor systems were characterized for their size, stability, and oxygen sensitivity *in vitro* and *in vivo*; and histological assessment of tissue reaction after administration was also conducted.

2. Materials and methods

2.1. Chemicals

All chemicals were purchased from Fluka unless specified and were all $\geq 99\%$ grade products. F15T-03 and F45T-03 were synthesized as described previously [29]. The hydrophilic trityl, CT-03, was kindly provided by HJ Halpern (University of Chicago).

2.2. Nano-emulsion preparation

F15T-03 and F45T-03 have different solubilities in PFC. F15T-03 was soluble in HFB and not in PFOB, while F45T-03 was soluble in both solvents. The highest concentration of the compounds was chosen according to their solubility in PFC and the need to avoid spin–spin exchange: F15T-03 1 mM in HFB and F45T-03 0.25 mM in PFOB. Solubilization was performed overnight. The solutions were filtered on a 0.2 μm GHP filter (Pall Acrodisc) before further manipulation. The nano-emulsions were prepared using 3-sn-phosphatidylcholine from dried egg yolk (purity $\geq 50\%$). 3-sn-phosphatidylcholine (3.120 g) was dispersed for 1 h in 100 ml PBS buffer. Eighteen (F15T-03/HFB nano-emulsion) or 16 (F45T-03/PFOB nano-emulsion) ml of the phospholipid dispersion were collected and further homogenized for 10 min with an Ultraturax (13,500 rpm). Two or 4 ml of the PFC solution (F15T-03 in HFB and FT45-03 in PFOB, respectively) containing the fluorinated trityl

were added drop by drop to the phospholipid dispersion. The emulsion was stirred for 30 min with the Ultraturax before being placed in an EmulsiFlex C-5 high-pressure homogenizer (Avestin) working at 20,000 psi for 12–20 min (20–35 passes) (adapted from [34]). Final concentrations were 0.1 μmol F15T-03/0.1 ml HFB/25 mg lecithin and 0.05 μmol F45T-03/0.2 ml PFOB/28 mg lecithin for 1 ml of nano-emulsion.

2.3. Size measurement

Particle size was assessed using a Zetasizer Nano ZS (Malvern). The nano-emulsions were diluted (10 times) in PBS buffer to obtain 1 ml for the measurement. Values are expressed as a mean of three measurements \pm standard deviation (SD).

2.4. *In vitro* EPR oximetry

As the oxygen solubility is temperature dependent, all *in vitro* and *in vivo* experiment were made at 37 °C. Calibration measurements (EPR LW as a function of the $p\text{O}_2$) were performed at 9.3 GHz with a Bruker EMX EPR spectrometer equipped with a variable temperature controller BVT-3000. The sample (nano-emulsion containing F15T-03 or FT45-03, or aqueous solution of the hydrophilic CT-03) was placed in a gas-permeable Teflon tube (0.625 mm inner diameter; 0.05 mm wall). This tube was folded twice at both ends and placed in a quartz tube open at both ends. Measurements were taken at 310 K and at 21% and 0% oxygen. The oxygen content in the gas was analyzed using a Servomex oxygen analyzer OA540. Typical spectrometer parameters were modulation amplitude less than one third of the peak-to-peak LW, and incident microwave power of 100 μW . The frequency modulation was set at 10 kHz for CT-03, and 100 kHz for the F15T-03 and FT45-03 nano-emulsions. A kinetics experiment was also performed to check that the phospholipid shell allowed equilibrium with the oxygen environment [31]. Air was flushed at 400 l/h into the EPR spectrometer cavity and a first spectrum was acquired. The flushing gas was then changed to N_2 and an EPR spectrum was recorded every minute. After equilibrium, the gas in the cavity was changed back to 21% oxygen.

2.5. *In vivo* EPR oximetry

Animal experiments were carried out in compliance with national care regulations and the local ethics committee (protocol 2004/UCL/MD/026). NMRI male mice (Janvier) and Wistar rats (Animalerie Facultaire, Université catholique de Louvain) were used for these experiments. The animals were anesthetized with isoflurane before administration of the nano-emulsions into the gastrocnemius muscle (150 μl in mice and 500 μl in rats). *In vivo* EPR spectra were recorded using an EPR spectrometer (Magnetech, Berlin, Germany) with a low-frequency microwave bridge operating at 1.2 GHz and an extended loop resonator. Local hypoxia was induced by restriction of the blood supply in the muscle; the base of the thigh was reversibly tied with an elastic band to restrict blood flow through the femoral arteries. Measurements ($n = 5$ per group) were carried out during normoxia (3 min after nano-emulsion injection) and 5 min after inducing ischemia. Infra-red lights have been used in order to maintain the temperature of the animals. Parameters for experiments with CT-03 were: center field: 53 mT; modulation amplitude: 0.00315 mT; modulation frequency: 10 kHz; power: 600 μW . For F15T-03 and F45T-03 nano-emulsions, the acquisition parameters were: center field: 53 mT; sweep width: 1.0 mT; modulation amplitude: 0.021 mT; modulation frequency: 100 kHz; power: 23.8 mW.

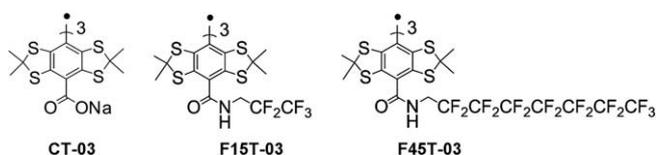


Fig. 1. Chemical structures of hydrophilic trityl CT-03, F15T-03 and FT45-03 fluorinated trityl.

2.6. Histological evaluation

The effect of the nano-emulsions on the muscle tissue was assessed by histological examination. Thirty microliters of F15T-03/HFB or F45T-03/PFOB were administered intramuscularly. Four or 24 h later, mice were sacrificed and the muscle into which the nano-emulsion had been administered was carefully removed. After fixing the samples ($n = 2$) in 10% formalin for 48 h, they were embedded in paraffin blocks and prepared into histological slices (5 μm thickness). Slices were stained using a classical hematoxylin–eosin procedure. Picture captions were taken using an optical microscope (Nikon Alphashot-2 Y52) (magnification 100 \times) and a digital photo camera, Nikon CoolPix 4500.

3. Results and discussion

3.1. Size measurement and stability of the nano-emulsions

The homogenizing procedure was critical in order to obtain a stable nano-emulsion. Without high-pressure homogenization, it was impossible to obtain a stable emulsion. After the nano-emulsion had been processed, particle size measurements were performed. The F15T-03/HFB nano-emulsion was characterized by an average diameter of 112 ± 1 nm and a polydispersity index (PDI) of 0.223 on the day of preparation. For the F45T-03/PFOB nano-emulsion, the average diameter was 182 ± 3 nm and the PDI 0.158. This distribution size would allow intravascular administration of these nano-emulsions. The size distribution remained stable for at least one month for the F15T-03/HFB nano-emulsion and two weeks for the F45T-03/PFOB nano-emulsion (data not shown).

3.2. In vitro EPR oximetry

When changing the oxygen environment, the nano-emulsions containing F15T-03/HFB and F45T-03/PFOB had larger variations in LW compared to the hydrophilic CT-03 trityl. The ΔLW s when changing from air to nitrogen were 0.2336 mT (0.0554 mT and 0.289 mT at 0% and 21% oxygen) for the F15T-03/HFB nano-emulsion, 0.0962 mT (0.0548 mT and 0.151 mT at 0% and 21% oxygen) for the F45T-03/PFOB nano-emulsion and 0.010 mT (0.009 mT and 0.019 mT at 0% and 21% oxygen) for the CT-03 aqueous solution. From these data, it is possible to calculate the % increase in LW compared to the values measured at 0% oxygen. The increase in LW were 521%, 275% and 211% for the nano-emulsion F15T-03/HFB the F45T-03/PFOB nano-emulsion and the CT-03 solution, respectively. These data demonstrate that both nano-emulsions have increased sensitivity to oxygen variation.

Interestingly, the LW equilibrium values in air were comparable for F15T-03 when dissolved in HFB or encapsulated in the nano-emulsions. However, the LW values obtained for F45T-03 were larger when this compound was dissolved in PFOB [29] than when it was encapsulated in PFOB (0.334 mT in PFOB versus 0.151 mT in the nano-emulsion). Importantly, the calibration (LW as a function of $p\text{O}_2$) remained stable over time (more than one week, data not shown). The kinetics experiment clearly showed that the phospholipid shell around the dispersed PFC nano-droplets was totally permeable to gaseous oxygen exchange. As shown in Fig. 2, the equilibrium of the nano-emulsion of F15T-03 with the gas environment was achieved within less than 5 min when changing from air to nitrogen and vice-versa.

3.3. In vivo EPR oximetry

After intramuscular administration of hydrosoluble CT-03 trityl or F15T-03 or F45T-03 nano-emulsions, the animals were placed in

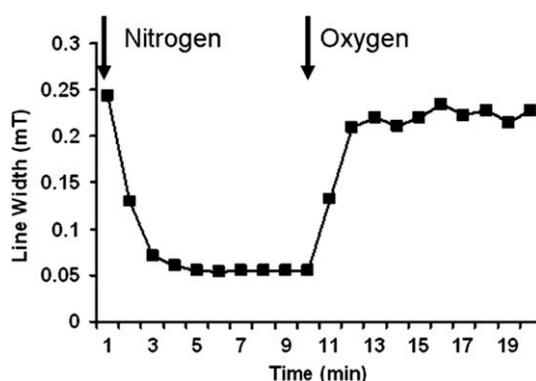


Fig. 2. Kinetic of fast oxygen exchanges in nano-emulsions of F15T-03. Nitrogen was flushed into the chamber for 10 min starting from time 0 (first arrow); at 11 min oxygen was flushed (second arrow).

our L-band EPR spectrometer. At this frequency, EPR can be carried out with a depth of penetration of about 1 cm, which is optimal for studies in rodents. The LWs (means \pm SD) observed in normoxic muscle were 0.0134 ± 0.0011 mT for the CT-03 solution, 0.092 ± 0.0044 mT and 0.079 ± 0.0025 mT for F15T-03 and F45T-03 nano-emulsions, respectively. These values correspond to $p\text{O}_2$ values (means \pm SD) of 70.3 ± 18.2 mmHg for the CT-03 solution, 25.0 ± 3.0 mm Hg and 40.8 ± 4.1 mm Hg for F15T-03 and F45T-03 nano-emulsions, respectively. These values are consistent with previously published data recorded in muscles of rodents anesthetized with isoflurane [32,33]. The differences between the two nano-emulsions are not significant in term of $p\text{O}_2$. The apparent discrepancy could come from the inflammatory reaction that has been observed with the use of the F15T-03/HFB nano-emulsion. The important standard deviation using CT-03 can be attributed to the limited resolution accuracy when measuring very small LW.

The variation in LW after interruption of blood flow was significantly lower with the hydrophilic CT-03 than with the nano-emulsions. The hydrophilic CT-03 solution had a ΔLW of 0.0038 ± 0.0023 mT, compared to 0.0208 ± 0.0096 mT and 0.0194 ± 0.0071 mT for F15T-03 and F45T-03, respectively (Fig. 3). This corresponds to a fivefold increase in sensitivity to oxygen variations in vivo. This increase in oxygen sensitivity is appreciable when monitoring subtle modulations of oxygen in vivo. However, a disadvantage of using nano-emulsions is the decrease in signal intensity obtained in vivo compared to the hydrophilic compound, CT-03. This is the result of three different phenomena: (1) an intrinsically larger LW even at low $p\text{O}_2$ (the signal intensity is inversely proportional to the square of the EPR LW); (2) the need

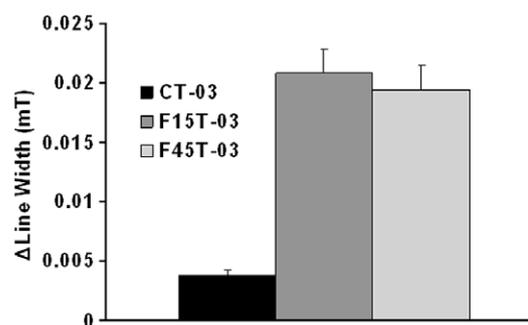


Fig. 3. In vivo ΔLW of measurement at normoxia and after leg ligation in mice injected with the trityl CT-03 (black columns), or the F15T-03/HFB nano-emulsion (dark gray columns), and rats injected with the F45T-03/PFOB nano-emulsion (light gray columns).

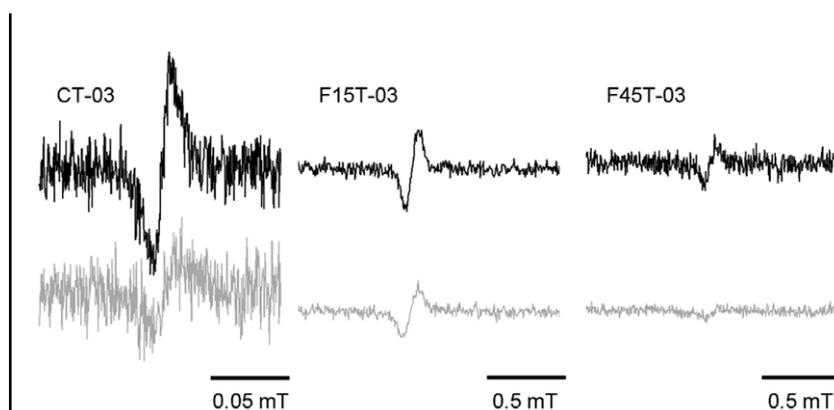


Fig. 4. In vivo spectrum of measurement at normoxia (gray) and after leg ligation (black). Left: CT-03; center: F15T-03/HFB; right: F45T-03/PFOB.

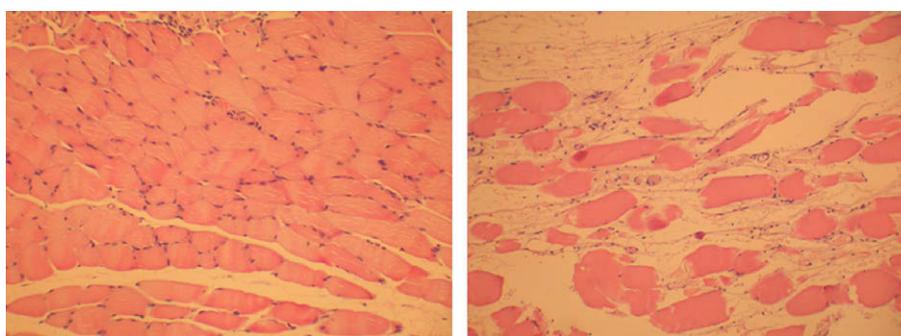


Fig. 5. Histological sections of muscles after administration of F45T-03/PFOB at 4 h (left) and F15T-03/HFB at 4 h (right).

to avoid a spin–spin exchange in the starting PFC solution (concentration < 5 mM); (3) the dilution factor when preparing an emulsion of PFC in water solutions. This difference in signal intensity is illustrated in Fig. 4.

3.4. Reactivity in tissues and histology

After intramuscular administration, the F15T-03/HFB emulsions rapidly produced edema in the muscle, but there was no visible reaction with the F45T-03/PFOB nano-emulsions. To better characterize this phenomenon, a preliminary histological examination was carried out. No inflammation was detected either at 4 or at 24 h after injection (Fig. 5, left panel) in mice which had received the F45T-03/PFOB nano-emulsion. This is in accordance with the considerable amount of work investigating the use of this PFC as a blood substitute [34]. The situation was different in the group that received F15T-03/HFB. As shown in Fig. 5 (right panel), an inflammatory process was observed after administration of this compound, characterized by considerable edema, eosinophilia, abnormalities in the muscle cell structure, and lack of cell nucleus. This situation persisted 24 h after administration of the nano-emulsion.

4. Conclusions

We have developed new systems that incorporate fluorine trityls in nano-emulsions containing PFC. These compounds were evaluated for their performance as EPR oxygen sensors. Stable formulations were achievable using high-pressure homogenization, and nano-emulsions were usable for at least two weeks after preparation. A large increase in sensitivity to oxygen was observed both

in vitro and in vivo when using these nano-emulsions compared to hydrophilic trityls. When comparing the two nano-emulsions, the F15T-03/HFB nano-emulsion had the highest sensitivity in vitro to oxygen variation. Moreover, its higher solubility (up to 1 mM in HFB) allowed preparation of a nano-emulsion detectable in vivo with a high signal-to-noise ratio. However, in vivo this compound induced an inflammatory reaction and edema. The F45T-03/PFOB nano-emulsion, while being apparently less efficient, is still five times more sensitive to oxygen than hydrophilic trityls. This formulation did not induce any inflammatory response in preliminary tests, and should be considered further as a system to monitor subtle changes in tissue oxygenation in vivo.

Acknowledgments

This work was supported by grants from the Belgian National Fund for Scientific Research (FNRS), the Fonds Joseph Maisin, the Saint-Luc Foundation, the “Actions de Recherches Concertées-Communauté Française de Belgique-ARC 04/09-317”, and the “Pôle d’attraction Interuniversitaire PAI VI (P6/38)”.

References

- [1] B. Gallez, C. Baudelet, B.F. Jordan, Assessment of tumor oxygenation by electron paramagnetic resonance: principles and applications, *NMR Biomed.* 17 (2004) 240–262.
- [2] J.L. Tatum, G.J. Kelloff, R.J. Gillies, J.M. Arbeit, J.M. Brown, K.S. Chao, J.D. Chapman, W.C. Eckelman, A.W. Fyles, A.J. Giaccia, R.P. Hill, C.J. Koch, M.C. Krishna, K.A. Krohn, J.S. Lewis, R.P. Mason, G. Melillo, A.R. Padhani, G. Powis, J.G. Rajendran, R. Reba, S.P. Robinson, S.G. Semenza, H.M. Swartz, P. Vaupel, D. Yang, B. Croft, J. Hoffman, G. Liu, H. Stone, D. Sullivan, Hypoxia: importance in tumor biology, noninvasive measurement by imaging, and value of its measurement in the management of cancer therapy, *Int. J. Radiat. Biol.* 82 (2006) 699–757.

- [3] D.S. Vikram, J.L. Zweier, P. Kuppusamy, Methods for noninvasive imaging of tissue hypoxia, *Antioxid. Redox. Signal.* 9 (2007) 1745–1756.
- [4] K.J. Liu, P. Gast, M. Moussavi, S.W. Norby, N. Vahidi, T. Walczak, M. Wu, H.M. Swartz, Lithium phthalocyanine: a probe for electron paramagnetic resonance oximetry in viable biological systems, *Proc. Natl. Acad. Sci. USA* 90 (1993) 5438–5442.
- [5] R.P. Pandian, N.L. Parinandi, G. Ilangoan, J.L. Zweier, P. Kuppusamy, Novel particulate spin probe for targeted determination of oxygen in cells and tissues, *Free Radic. Biol. Med.* 35 (2003) 1138–1148.
- [6] N. Vahidi, R.B. Clarkson, K.J. Liu, S.W. Norby, M. Wu, H.M. Swartz, In vivo and in vitro EPR oximetry with fusicite: a new coal-derived, particulate EPR probe, *Magn. Reson. Med.* 31 (1994) 139–146.
- [7] P.E. James, O.Y. Grinberg, F. Goda, T. Panz, J.A. O'Hara, H.M. Swartz, Gloxy: an oxygen-sensitive coal for accurate measurement of low oxygen tensions in biological systems, *Magn. Reson. Med.* 38 (1997) 48–58.
- [8] B.F. Jordan, C. Baudelet, B. Gallez, Carbon-centered radicals as oxygen sensors for in vivo electron paramagnetic resonance. screening for an optimal probe among commercially available charcoals, *MAGMA* 7 (1998) 121–129.
- [9] B. Gallez, B.F. Jordan, C. Baudelet, P.D. Misson, Pharmacological modifications of the partial pressure of oxygen in murine tumors: evaluation using in vivo EPR oximetry, *Magn. Reson. Med.* 42 (1999) 627–630.
- [10] H.M. Swartz, K.J. Liu, F. Goda, T. Walczak, India ink: a potential clinically applicable EPR oximetry probe, *Magn. Reson. Med.* 31 (1994) 229–232.
- [11] F. Goda, K.J. Liu, T. Walczak, J.A. O'Hara, J. Jiang, H.M. Swartz, In vivo oximetry using EPR and India ink, *Magn. Reson. Med.* 33 (1995) 237–245.
- [12] M. Lan, N. Beghein, N. Charlier, B. Gallez, Carbon blacks as EPR sensors for localized measurements of tissue oxygenation, *Magn. Reson. Med.* 51 (2004) 1272–1278.
- [13] B. Gallez, R. Debuyst, R. Demeure, F. Dejehet, C. Grandin, B. Van Beers, H. Taper, J. Pringot, P. Dumont, Evaluation of a nitroxyl fatty acid as liver contrast agent for magnetic resonance imaging, *Magn. Reson. Med.* 30 (1993) 592–599.
- [14] B. Gallez, V. Lacour, R. Demeure, R. Debuyst, F. Dejehet, J.L. De Keyser, P. Dumont, Spin labelled arabinogalactan as MRI contrast agent, *Magn. Reson. Imaging* 12 (1994) 61–69.
- [15] J.H. Ardenkjaer-Larsen, I. Laursen, I. Leunbach, G. Ehnholm, L.G. Wistrand, J.S. Petersson, K. Golman, EPR and DNP properties of certain novel single electron contrast agents intended for oximetric imaging, *J. Magn. Reson.* 133 (1998) 1–12.
- [16] S. Subramanian, K. Yamada, A. Irie, R. Murugesan, J.A. Cook, N. Devasahayam, G.M. Van Dam, J.B. Mitchell, M.C. Krishna, Noninvasive in vivo oximetric imaging by radiofrequency FT EPR, *Magn. Reson. Med.* 47 (2002) 1001–1008.
- [17] K. Matsumoto, S. Subramanian, N. Devasahayam, T. Aravalluvan, R. Murugesan, J.A. Cook, J.B. Mitchell, M.C. Krishna, Electron paramagnetic resonance imaging of tumor hypoxia: enhanced spatial and temporal resolution for in vivo pO_2 determination, *Magn. Reson. Med.* 55 (2006) 1157–1163.
- [18] M. Elas, K.H. Ahn, A. Parasca, E.D. Barth, D. Lee, C. Haney, H.J. Halpern, Electron paramagnetic resonance oxygen images correlate spatially and quantitatively with Oxlyte oxygen measurements, *Clin. Cancer Res.* 12 (2006) 4209–4217.
- [19] A.A. Bobko, I. Dhimitruka, J.L. Zweier, V.V. Khramtsov, Trityl radicals as persistent dual function pH and oxygen probes for in vivo electron paramagnetic resonance spectroscopy and imaging: concept and experiment, *J. Am. Chem. Soc.* 129 (2007) 7240–7241.
- [20] I. Dhimitruka, A.A. Bobko, C.M. Hadad, J.L. Zweier, V.V. Khramtsov, Synthesis and characterization of amino derivatives of persistent trityl radicals as dual function pH and oxygen paramagnetic probes, *J. Am. Chem. Soc.* 130 (2008) 10780–10787.
- [21] B.B. Williams, H. al Hallaq, G.V. Chandramouli, E.D. Barth, J.N. Rivers, M. Lewis, V.E. Galtsev, C.S. Karczmar, H.J. Halpern, Imaging spin probe distribution in the tumor of a living mouse with 250 MHz EPR: correlation with BOLD MRI, *Magn. Reson. Med.* 47 (2002) 634–638.
- [22] M.C. Krishna, S. English, K. Yamada, J. Yoo, R. Murugesan, N. Devasahayam, J.A. Cook, K. Golman, J.H. Ardenkjaer-Larsen, S. Subramanian, J.B. Mitchell, Overhauser enhanced magnetic resonance imaging for tumor oximetry: coregistration of tumor anatomy and tissue oxygen concentration, *Proc. Natl. Acad. Sci. USA* 99 (2002) 2216–2221.
- [23] H. Li, Y. Deng, G. He, P. Kuppusamy, D.J. Lurie, J.L. Zweier, Proton electron double resonance imaging of the in vivo distribution and clearance of a triaryl methyl radical in mice, *Magn. Reson. Med.* 48 (2002) 530–534.
- [24] K.J. Liu, M.W. Grinstaff, J. Jiang, K.S. Suslick, H.M. Swartz, W. Wang, In vivo measurement of oxygen concentration using sonochemically synthesized microspheres, *Biophys. J.* 67 (1994) 896–901.
- [25] V. Dang, J. Wang, S. Feng, C. Buron, F.A. Villamena, P.G. Wang, P. Kuppusamy, Synthesis and characterization of a perchlorotriphenylmethyl (trityl) triester radical: a potential sensor for superoxide and oxygen in biological systems, *Bioorg. Med. Chem. Lett.* 17 (2007) 4062–4065.
- [26] J.Z. Sostaric, R.P. Pandian, A. Bratasz, P. Kuppusamy, Encapsulation of a highly sensitive EPR active oxygen probe into sonochemically prepared microspheres, *J. Phys. Chem. B* 111 (2007) 3298–3303.
- [27] P. Kirsch, in: Wiley-Vch Verlag GmbH & Co (Eds.), *Modern Fluoroorganic Chemistry, Synthesis, Reactivity, Applications*, Weinheim, 2004, p. 264.
- [28] A.A. Hirata, D.H. Sussdorf, Immunogenicity of insolubilized bovine serum albumin, *J. Immunol.* 96 (1966) 611–613.
- [29] B. Driesschaert, N. Charlier, B. Gallez, J. Marchand-Brynaert, Synthesis of two persistent fluorinated tetrathiatriarylmethyl (TAM) radicals for biomedical EPR applications, *Bioorg. Med. Chem. Lett.* 18 (2008) 4291–4293.
- [30] I.T. Horvath, Fluorous biphasic chemistry, *Acc. Chem. Res.* 31 (1998) 641–650.
- [31] M. Dinguizli, S. Jeumont, N. Beghein, J. He, T. Walczak, P.N. Lesniewski, H. Hou, O.Y. Grinberg, A. Sucheta, H.M. Swartz, H.M. B. Gallez, Development and evaluation of biocompatible films of polytetrafluoroethylene polymers holding lithium phthalocyanine crystals for their use in EPR oximetry, *Biosens. Bioelectron.* 21 (2006) 1015–1022.
- [32] B.F. Jordan, J.Z. Kimpalou, N. Beghein, C. Dessy, O. Feron, B. Gallez, Contribution of oxygenation to BOLD contrast in exercising muscle, *Magn. Reson. Med.* 52 (2004) 391–396.
- [33] C. Baudelet, B. Gallez, Effect of anesthesia on the signal intensity in tumors using BOLD-MRI: comparison with flow measurements by Laser Doppler flowmetry and oxygen measurements by luminescence-based probes, *Magn. Reson. Imaging* 22 (2004) 905–912.
- [34] J.G. Riess, Understanding the fundamentals of perfluorocarbons and perfluorocarbons emulsions relevant to in vivo oxygen delivery, *Artif. Cells Blood Substit. Immobil. Biotechnol.* 33 (2005) 47–63.